


# VIDAS LIS


## Detection and confirmation of *Listeria* spp

Protocol validated by AFNOR n° BIO-12/2-06/94 for all food products and environment

### 1 detection using VIDAS LIS

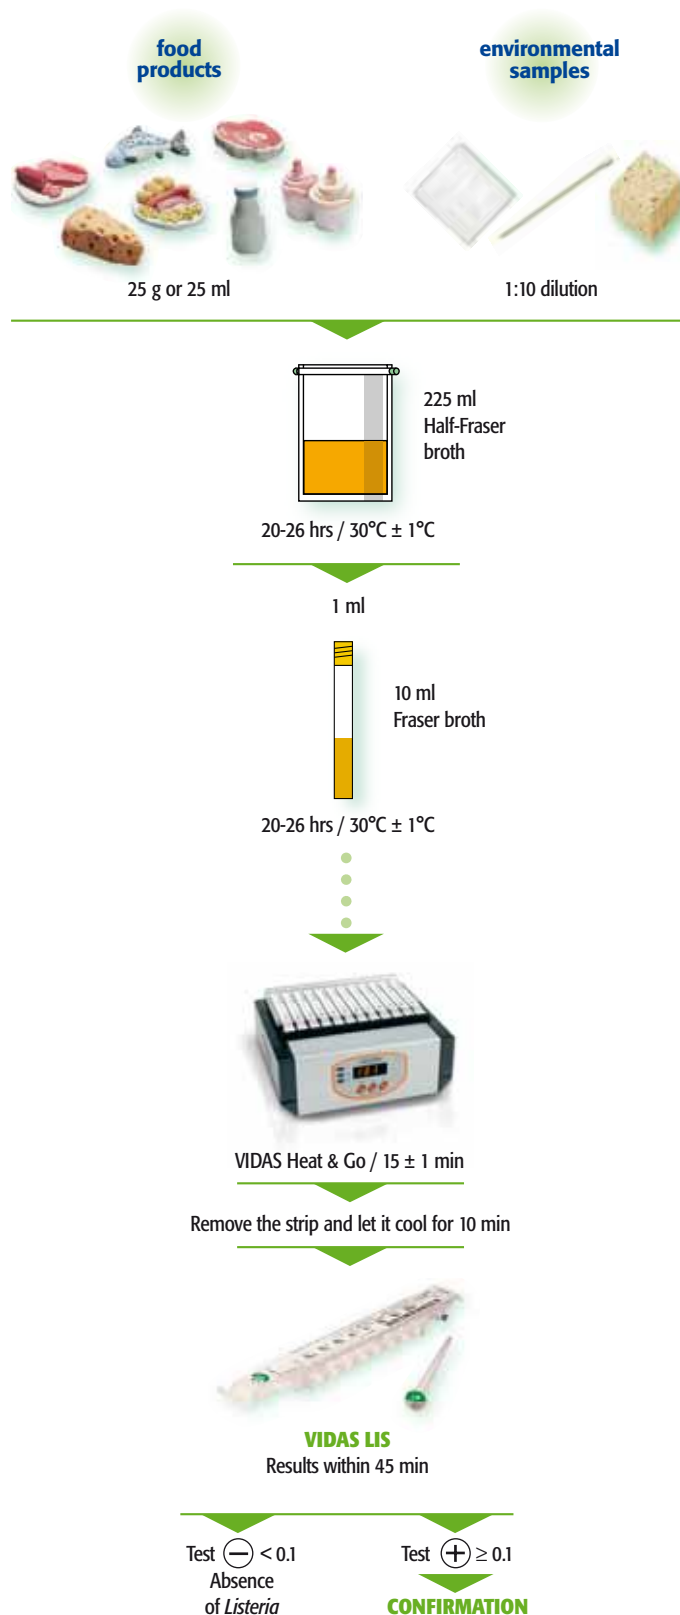

### 2 confirmation with reference method

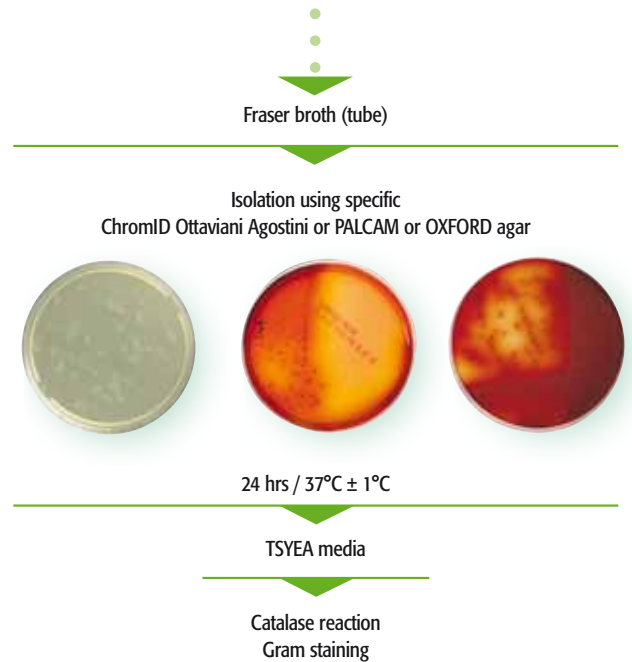

#### Listeria range

42615	Half-Fraser broth (Bottle 300 ml)	4 x 225 ml
42048	Half-Fraser broth (Bottle 250 ml)	6 x 225 ml
42112	Half-Fraser broth	20 tubes 10 ml
42627	Half-Fraser broth	3 x 3 l
42727	Half-Fraser broth (Minibags)	10 x 225 ml
42072	Fraser broth	20 tubes 10 ml
43559	Palcam agar	20 plates
43560	Oxford agar	20 plates
43641	ChromID Ottaviani Agostini Agar	20 plates
30700	VIDAS Listeria (LIS)	60 tests

For further details, consult the product package insert.



bioMérieux S.A.  
69280 Marcy l'Etoile  
France  
Tel. (33) 04 78 87 20 00  
Fax (33) 04 78 87 20 90

[www.biomerieux.com](http://www.biomerieux.com)  
[www.biomerieux-industry.com](http://www.biomerieux-industry.com)